

FIG. 1.

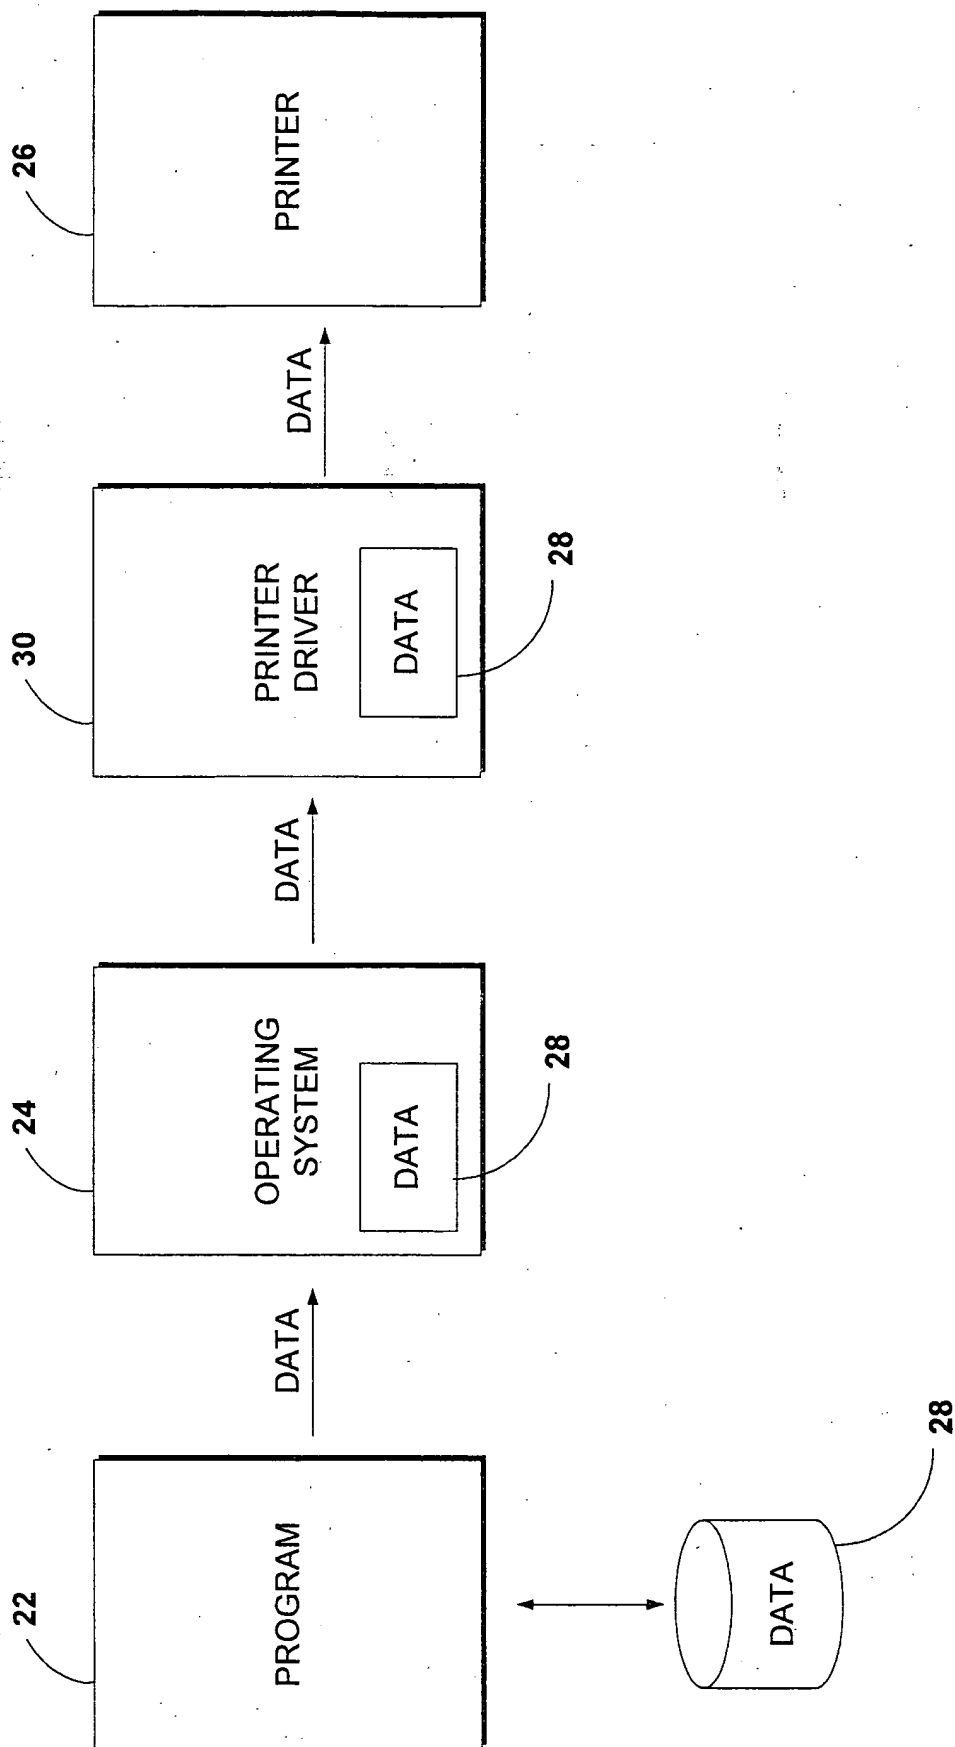


FIG. 2.

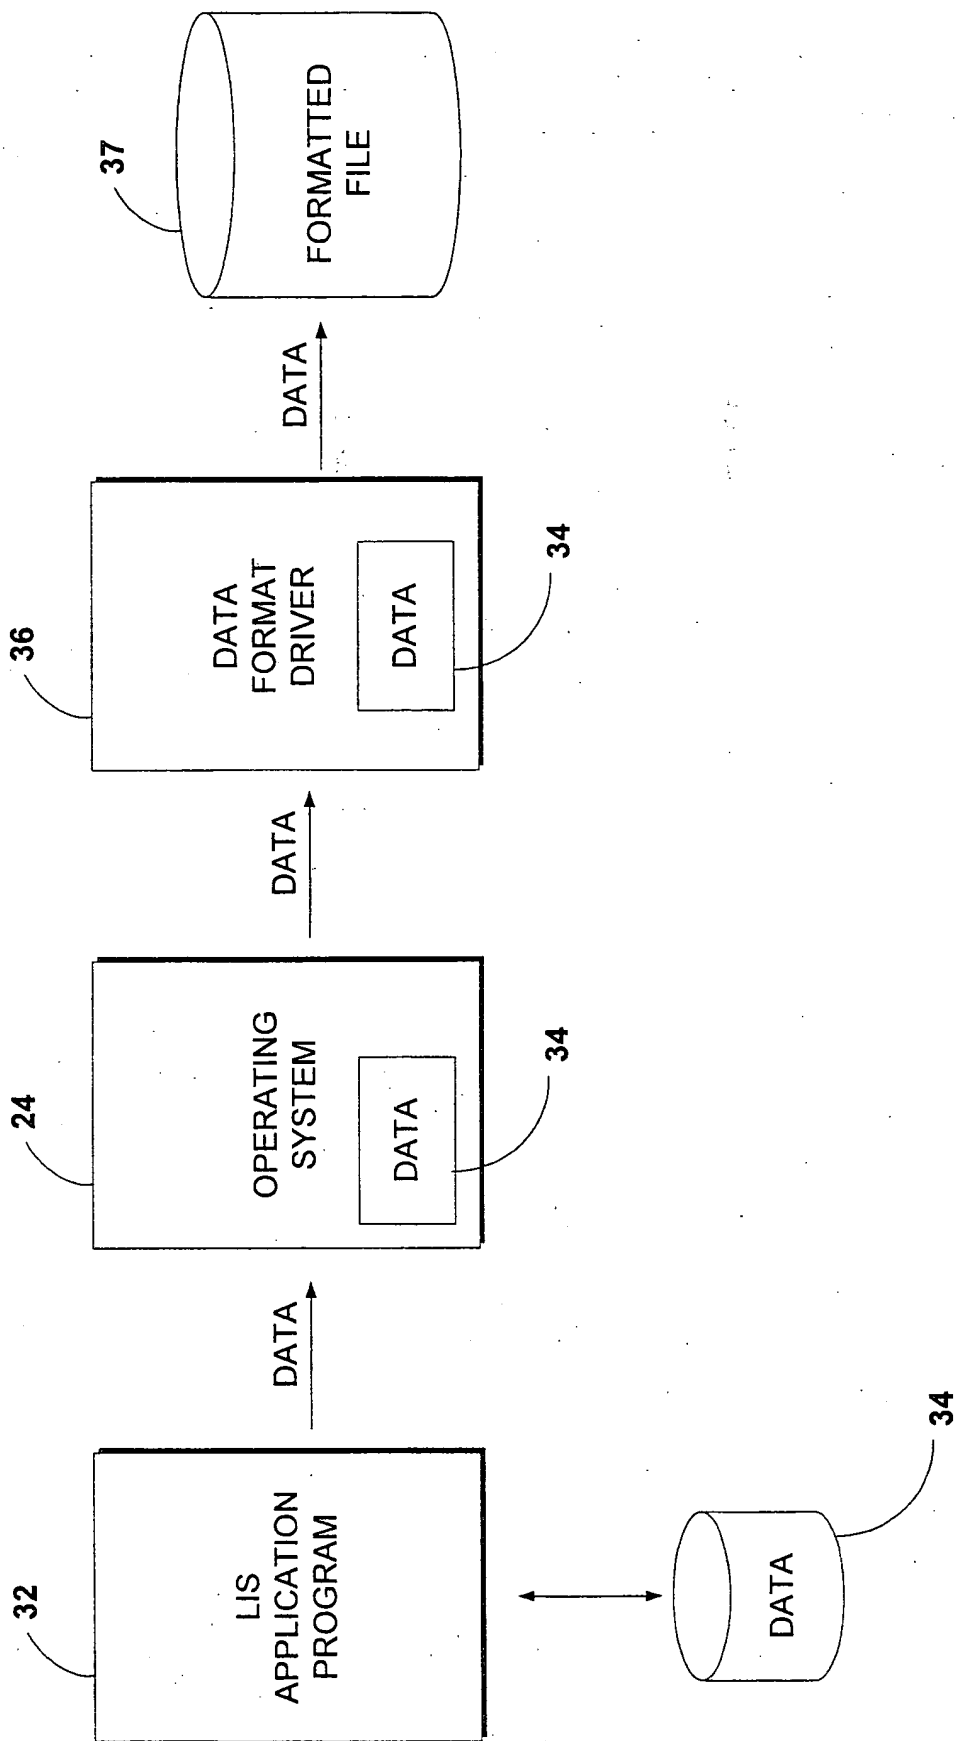


FIG. 3.

CONTROL MATERIAL QC		LEVEL	LOT #
DATE	TIME	TEST RESULT	UNIT
DATE	TIME	TEST RESULT	UNIT

38

40

42

44

46

48

50

52

54

FIG. 4.

HEMATRONIX	LIQUIDCHEM	LEVEL 1	LOT # 1116
01/01/2000	8:43 AM	GLUCOSE	120 mg/dL
01/02/2000	8:23 AM	GLUCOSE	122 mg/dL
01/03/2000	8:01 AM	GLUCOSE	122 mg/dL
01/04/2000	8:17 AM	GLUCOSE	119 mg/dL

56

58

58

58

58

FIG. 5.

LOT #	INSTRUMENT	TEST	DATE	TIME	RESULT	UNIT
-------	------------	------	------	------	--------	------

Diagram labels and their corresponding parts:

- 60: Points to the first row of the table.
- 62: Points to the 'LOT #' header.
- 64: Points to the 'INSTRUMENT' header.
- 66: Points to the 'TEST' header.
- 70: Points to the 'TIME' header.
- 72: Points to the 'RESULT' header.
- 74: Points to the 'UNIT' header.

FIG. 6.

1116	H747	GLUCOSE	120 mg/dL
1116	H747	GLUCOSE	122 mg/dL
1116	H747	GLUCOSE	122 mg/dL
1116	H747	GLUCOSE	119 mg/dL

76

FIG. 7.

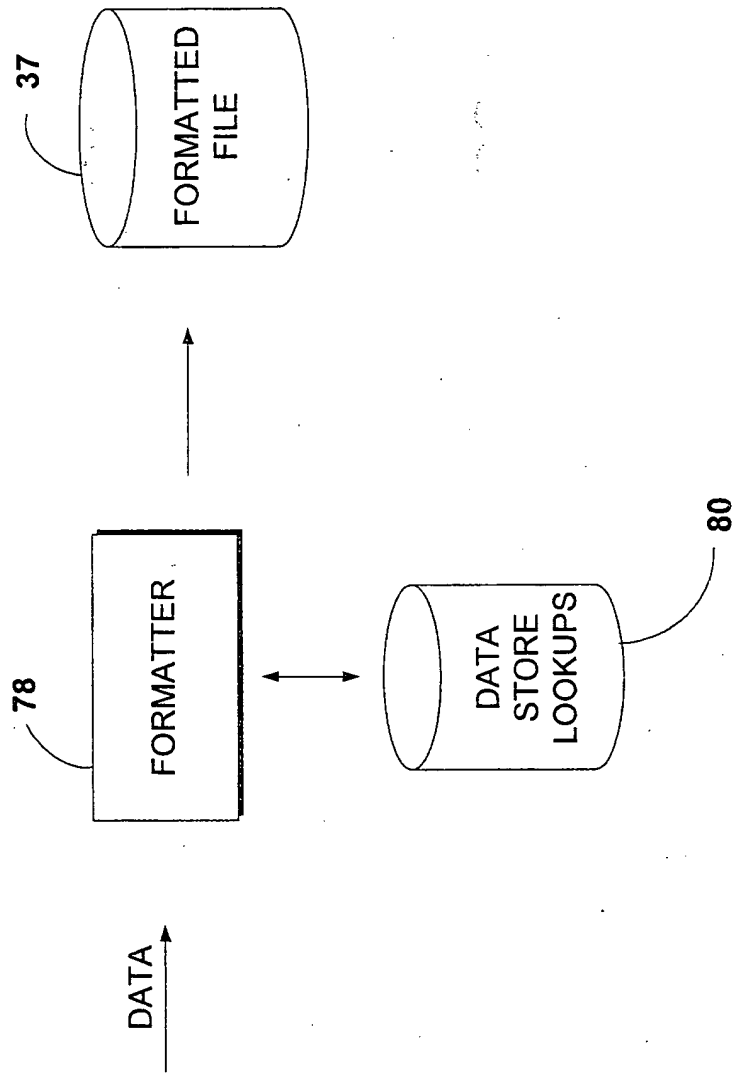


FIG. 8.

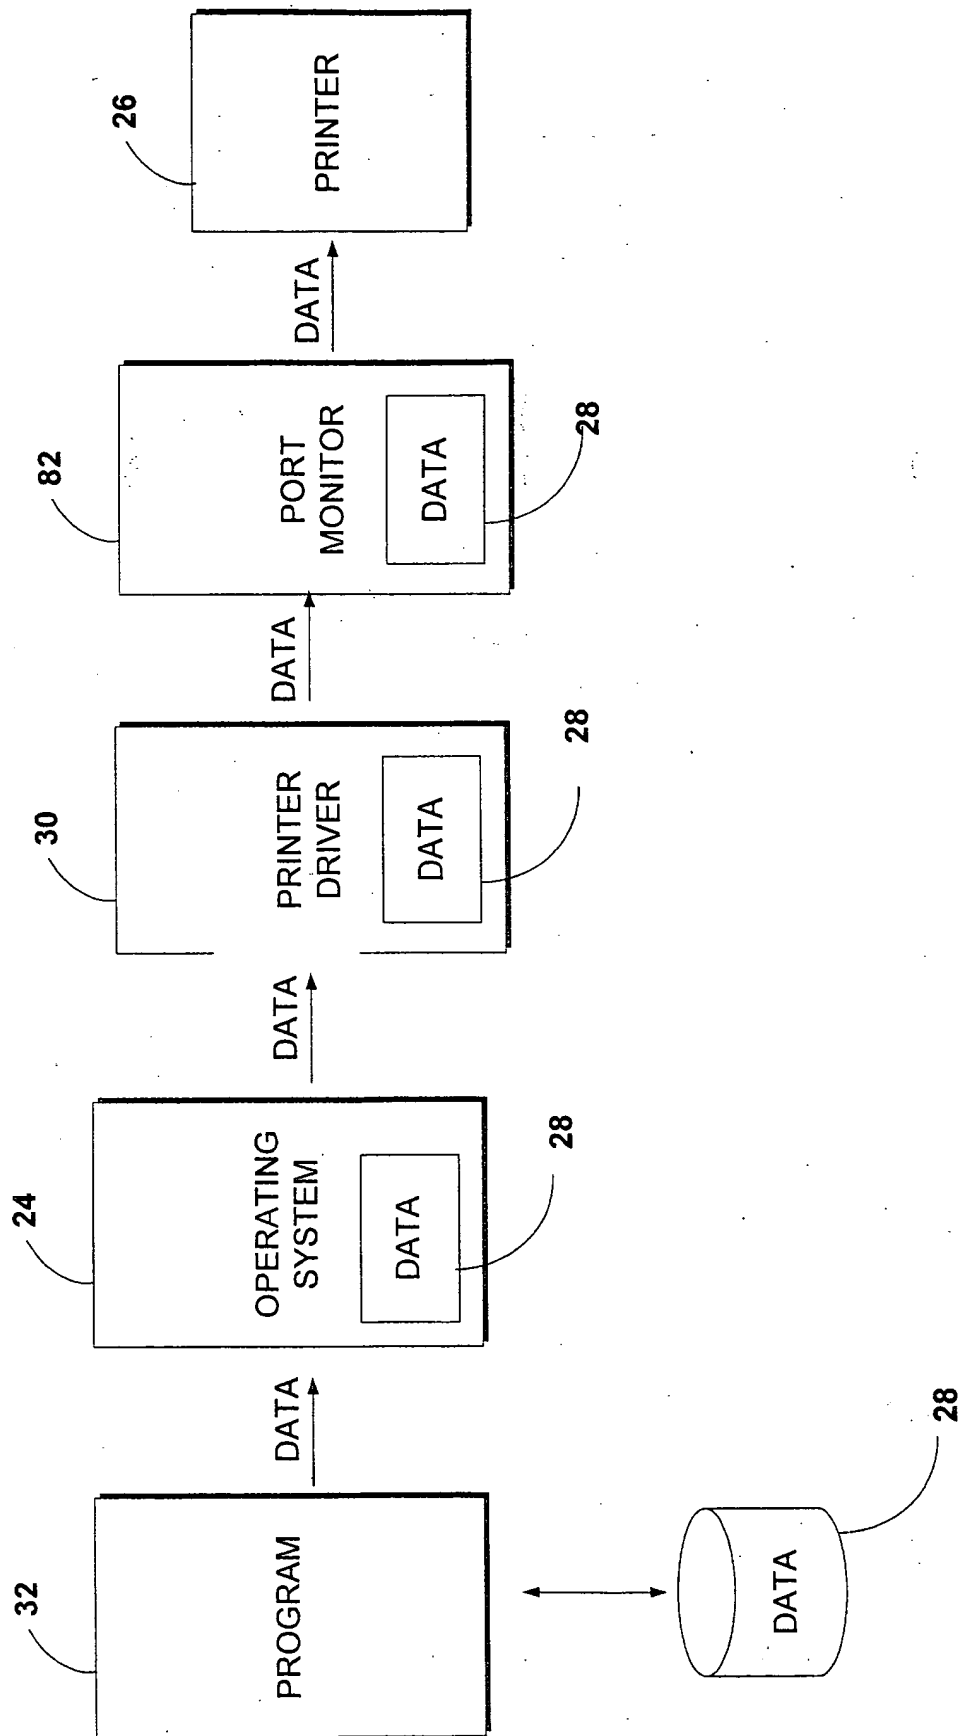


FIG. 9.

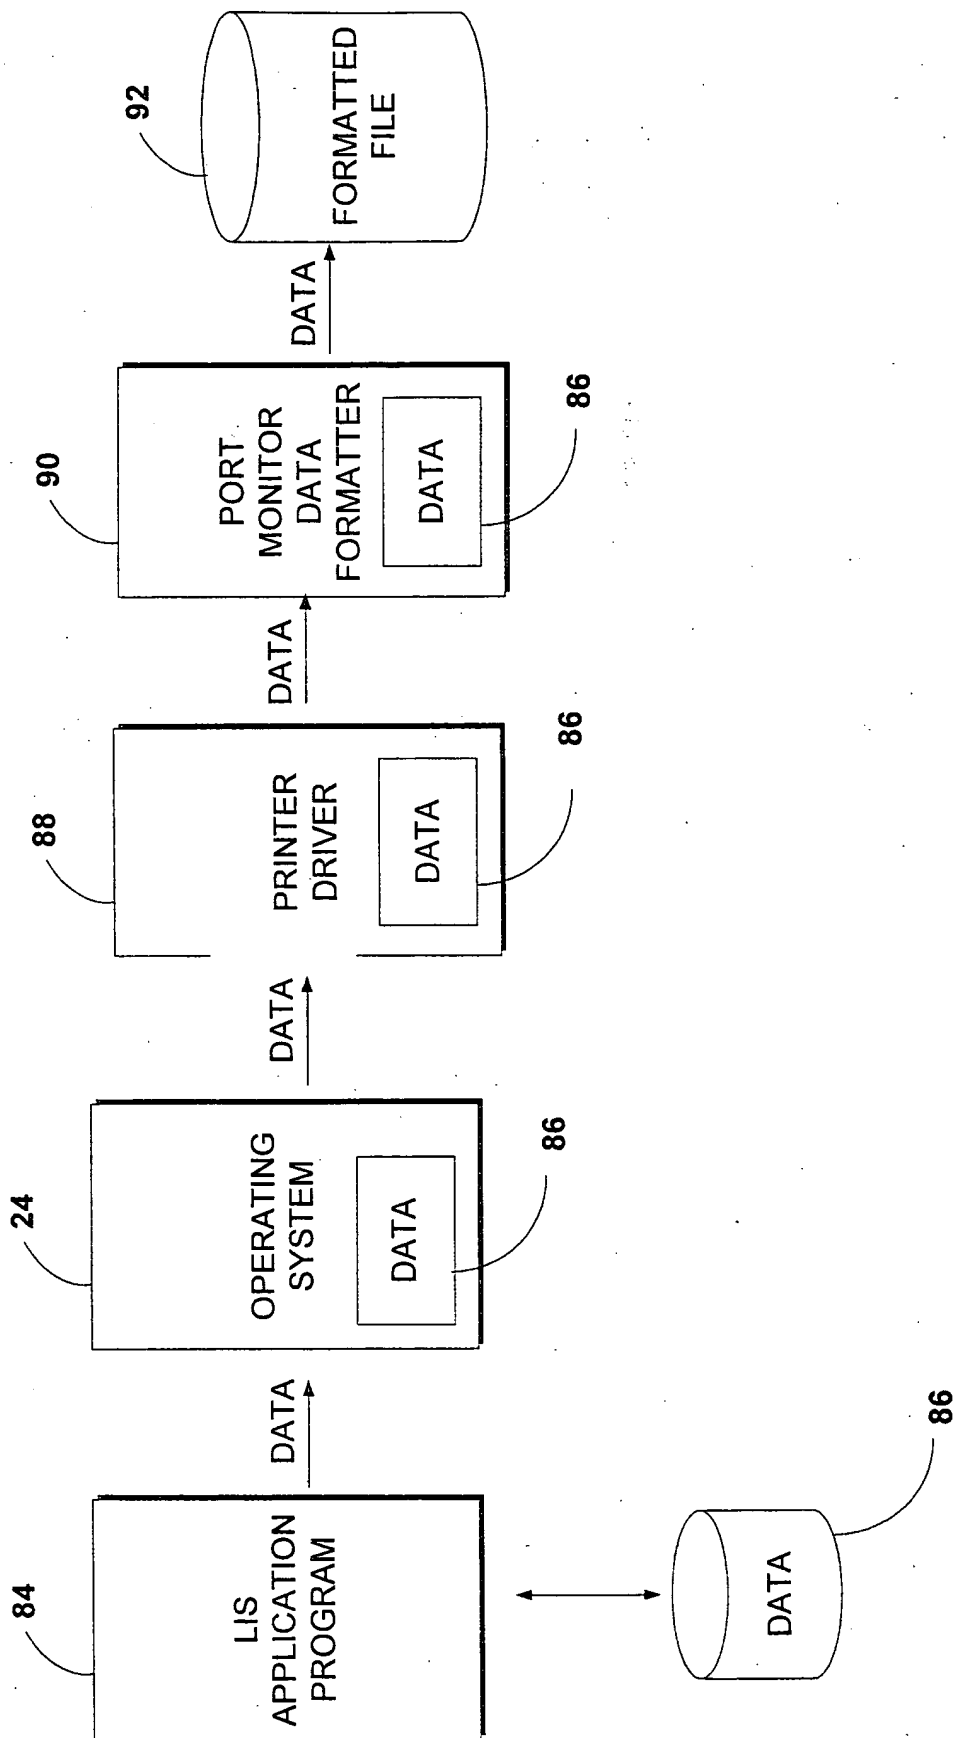


FIG. 10.